

FIG. 4 is a perspective view of the apparatus of FIG. 1, showing the apparatus in a retracted position.

FIG. 4

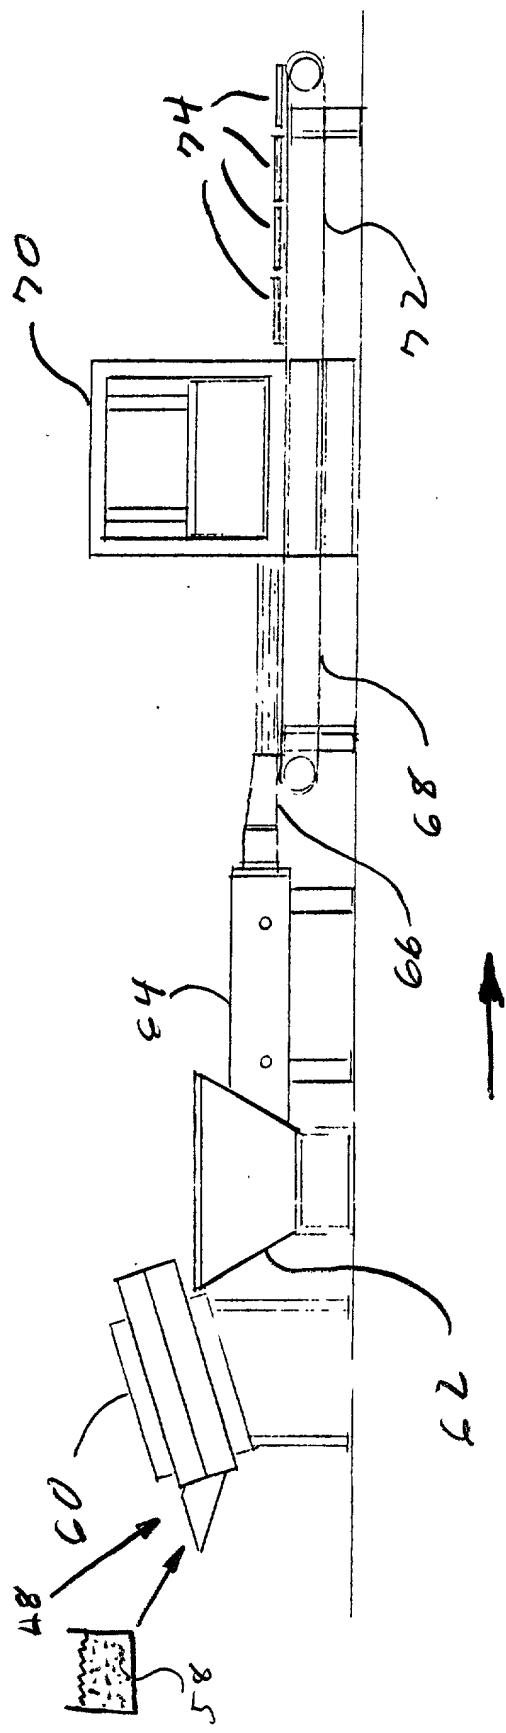


FIG. 5

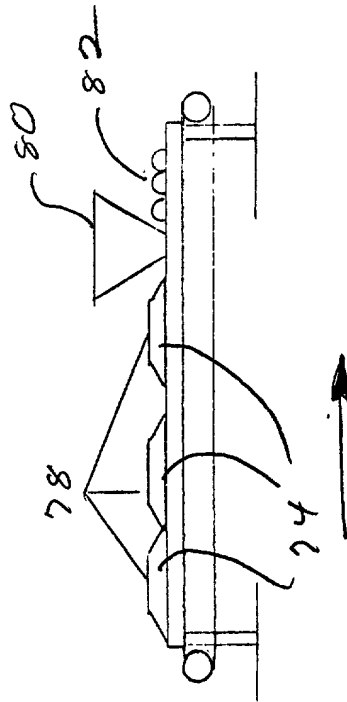
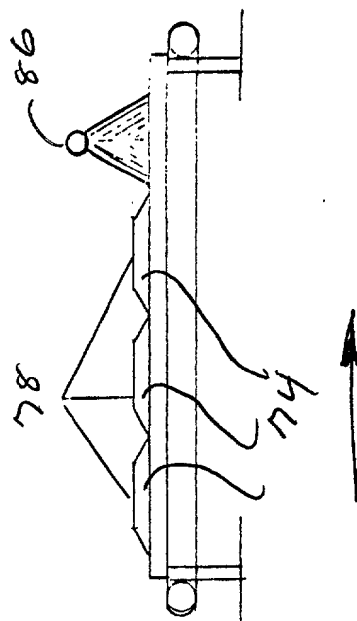


FIG. 6



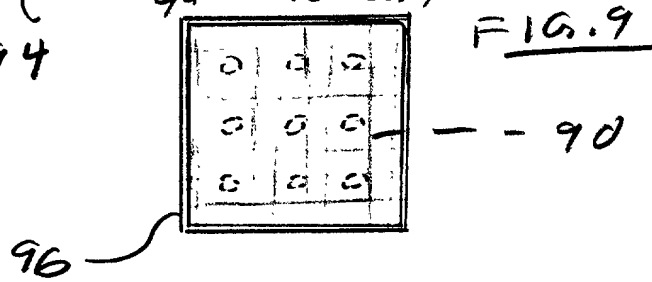
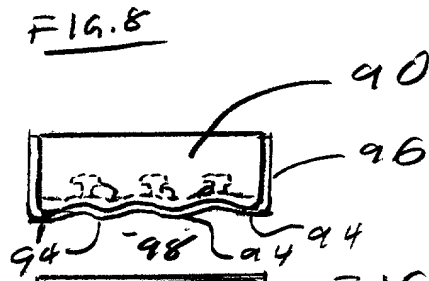
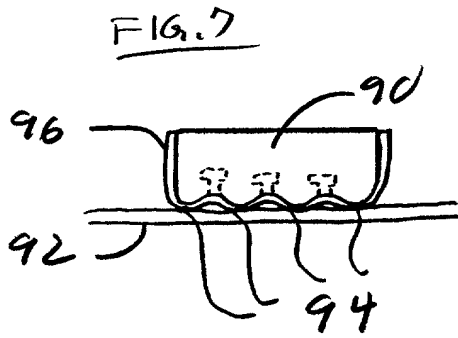




FIG. 11 is a perspective view of the device 100 in a closed position, showing the housing 140 and the lid 141. The device 100 is shown in a closed position, with the lid 141 covering the housing 140. The device 100 is shown in a perspective view, with the housing 140 and the lid 141. The device 100 is shown in a closed position, with the lid 141 covering the housing 140. The device 100 is shown in a perspective view, with the housing 140 and the lid 141.

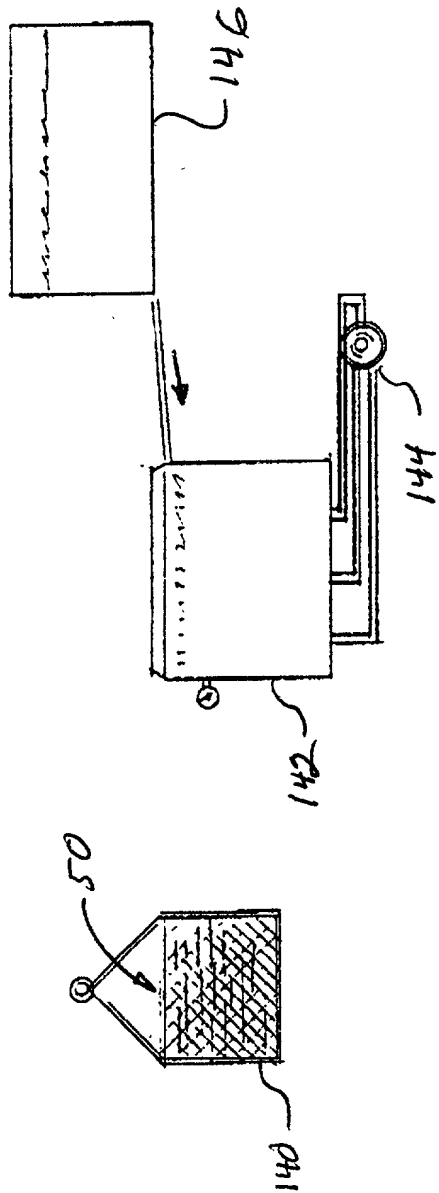


FIG. 11

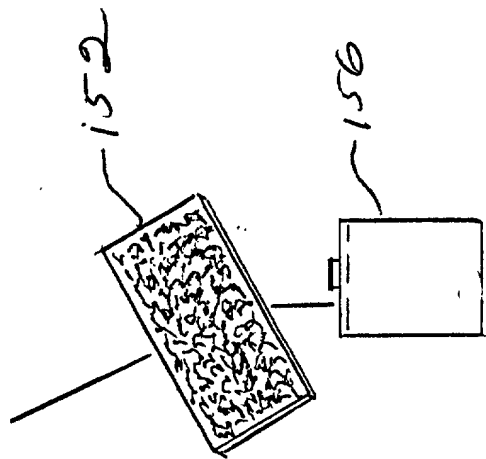


FIG. 12

154


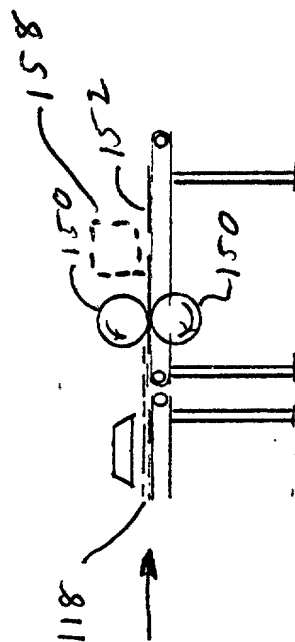


FIG. 13

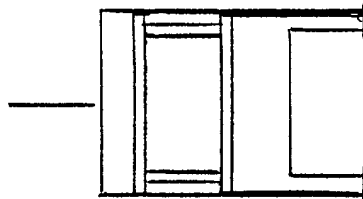